

Operating Instructions



Elmasonic xtra TT

Ultrasonic Cleaning Units



• english •

Contents

General.....	4
1 Important safety warnings	4
1.1 Instructions for the use of the present manual.....	4
1.2 Instructions for the use of the unit.....	5
1.3 Intended use as medical device	6
1.4 Safety instructions on the machine.....	6
2 Functioning.....	7
2.1 Ultrasonic cleaning factors.....	7
3 Product description.....	8
3.1 Elmasonic xtra TT product features.....	8
3.2 CE conformity	8
3.3 RFI Statement (European Union)	9
3.4 Delivered equipment.....	9
3.5 Unit front view / side view	10
3.6 Unit back view.....	11
3.7 Ball valve for draining the tank.....	11
3.8 Description of operating elements	12
3.9 Description of LED indicators	13
3.10 Operating and display functions	14
4 Initial operation	16
4.1 Connecting the unit to the mains	16
5 Putting unit into operation.....	17
5.1 Filling of the unit.....	17
5.2 Placement of cleaning items.....	18
5.3 Degassing of liquid	18
6 Ultrasonic cleaning process.....	19
6.1 Heating up of the cleaning liquid (units with heating).....	20
6.2 Starting the cleaning process manually	21
6.3 Sweep function	21
6.4 Activate dynamic function	22
6.5 Programme temperature limit	22
6.6 After the cleaning.....	23
7 Cleaning media	24
7.1 Limitations of use of cleaners containing solvents..	24
7.2 Limitations on aqueous cleaners	25
7.3 List of recommended cleaning media	25

7.3.1	Dental	26
7.3.2	Medical	26
7.3.3	Optics	26
7.3.4	Laboratory	27
7.3.5	Jewellery	27
7.3.6	Watches	27
7.3.7	Industry and workshop	28
8	Maintenance	29
8.1	Maintenance / Care	29
8.2	Service life of the transducer tank	29
8.3	Repair	30
9	Technical Details	31
10	Troubleshooting.....	33
11	Putting out of action and waste disposal	35
12	Manufacturer's contact address.....	35

General

The present Operating Instructions are part of the delivered equipment. They must be ready for use at any time and remain with the unit in case of resale.

We reserve the right to carry out technical modifications on the unit due to advanced development.

An operating manual cannot take account of every conceivable use. An operating manual cannot take account of every possible use. Contact your dealer or the manufacturer for further information or in the event of problems which are not covered or not sufficiently covered in this operating manual.

1 Important safety warnings

Please observe any additional national safety regulations that may apply.

1.1 Instructions for the use of the present manual

Carefully read the Operating Instructions before you operate the unit. Do not use the present electrical unit for any purpose other than described in the Operating Instructions.

Warning symbols used in the present manual:



This symbol warns of the risk of injury caused by electricity.



This symbol warns of the risk of injury caused by explosion and/or deflagration.



This symbol warns of the risk of injury caused by hot surfaces and liquids.



This symbol warns of the risk of injury.



This symbol warns of the risk of damage to the equipment.



This symbol marks additional information.

Signal words used in the present manual

Danger The signal word Danger warns of a potential risk of serious injury and danger to life.

Warning The signal word Warning warns of the risk of serious injury and heavy damage to the equipment.

Caution The signal word Caution warns of the risk of light injury or damage to the equipment.

Attention The signal word Attention warns of the risk of damage to the equipment.

1.2

Instructions for the use of the unit

Intended use	The present Elma ultrasonic cleaning unit has been designed for the treatment of items and liquids only. No cleaning of living beings or plants!
User	Operation of the unit by authorized and instructed staff only. Observe the instructions given in the manual.
Mains connection	For safety reasons, the present unit must be connected to a correctly grounded socket only. The technical details indicated on the nameplate must correspond with the available mains connection details, in particular those of the mains voltage and current connected value.
Prevention of electrical accidents	For purposes of maintenance and care of the unit, in the case of suspected humidity inside the unit or in the case of malfunctions and after operation, unplug the mains plug. The unit must only be opened by authorised specialised personnel.
Cleaning liquid	Fill the unit with a sufficient quantity of cleaning liquid before switch-on. Flammable liquids must not be treated by ultrasound directly in the cleaning tank: risk of fire and explosion!
Hot surfaces and liquids	Risk of burning and scalding! Depending on the operational period of the unit, unit surfaces, cleaning liquid, basket and cleaning items can heat up considerably.
Noise emission	Ultrasonic units can produce annoying sounds. Wear personal ear protection devices when working close to an ultrasonic unit which is operated without cover.
Sound transmission at physical contact	Do not reach inside the cleaning liquid or touch sound-carrying parts (tank, basket, cleaning items, etc.) during operation.
Exclusion of liability	The manufacturer cannot be held liable for damages on persons, equipment or cleaning items caused by improper use. The operator is responsible for the instruction of the operating staff.
Storage and transport conditions	Temperature during storage: +5 C (+41 F) to +40 C (+104 F) Temperature during transport: -15 C (+5 F) to +60 C (+140 C) Humidity and air pressure during storage and transport: 10 % - 80 % relative humidity; non-condensing Pressure range 500 hPa – 1060 hPa absolute

1.3 Intended use as medical device

Intended purpose Ultrasonic pre-cleaning of

- surgical and medical instruments
- micro instruments and
- rigid endoscopes and accessories

Only reusable medical devices that are approved for ultrasonic cleaning and authorised for the reprocessing are permitted to be cleaned (see information of the medical device manufacturer according to, e.g. EN ISO 17664).

The pre-cleaning of medical devices with Elmasonic xtra TT-Line products does not replace the subsequent cleaning, disinfection or sterilisation in automated standard processes (e.g. cleaning and disinfection unit (CDU) or autoclave).

The user is responsible for checking the cleaning result.

Intended use Ultrasonic cleaning machines are exclusively intended for ultrasonic irradiation of objects and liquids. Thereby, no flammable liquids are permitted to be used directly in the cleaning tanks.

The machine is only permitted to be operated by trained personnel and not by children. Operation and placement must be performed in accordance with the conditions and media defined in the operating manual.

The service intervals and regional regulations for checking the equipment must be complied with.

1.4 Safety instructions on the machine



Observe operating instructions!



Observe warnings and safety instructions given in the operating manual!



This symbol warns about the risk of injury from hot surfaces and liquids.



The unit cannot be disposed with household waste! Observe regional waste regulations!

2

Functioning

Today, cleaning by ultrasound is the most modern fine cleaning method.

The electric high-frequency energy created by an ultrasonic generator is transformed into mechanical energy by piezo-electrical transducer systems and is then transmitted into the bath.

This process creates millions of tiny vacuum bubbles which implode due to the variations of pressure caused by the ultrasonic activity. Highly energetic liquid jets are created. These jets remove dirt particles from surfaces and even from the smallest grooves and bores.

2.1

Ultrasonic cleaning factors



Mechanical energy

Basically, the cleaning result depends on four factors:

Ultrasonic energy is probably the most important mechanical factor in the cleaning process. This energy must be transmitted through a liquid medium to the surfaces which are to be cleaned. The present Elmasonic unit is fitted with the innovative sweep function device: electronic oscillation of the sound field (sweep function) prevents the formation of zones of low performance in the ultrasonic bath.

Cleaning media

For saponification and removal of the dirt particles a suitable cleaning agent is required. Elma has a large range of cleaning media on offer.

Cleaning chemicals are also necessary to reduce the surface tension. This increases considerably the efficiency of the ultrasonic activity.

Temperature

The effect of the cleaning medium is improved by the optimised temperature of the cleaning liquid.

For Elma cleaning products please observe the instructions given on the label or the product information leaflets.

Cleaning period

The cleaning period depends on the degree and the kind of contamination and on the correct selection of ultrasonic energy, cleaning agent and temperature.

3 Product description

3.1 Elmasonic xtra TT product features

- efficient 37 kHz ultrasonic high-performance transducers
- cleaning tank made of cavitation-resistant stainless steel
- user-friendly and clearly arranged operating panel; sealed against liquid intrusion to protect the electronics
- LED display for ultrasonic function
- rotary switch for easy preselection of the cleaning line
- continuous operating or short-term operation between 1 and 30 minutes
- permanent sweep function for optimized sound field distribution through frequency modulation
- Switchable Dynamic-function increases the peak ultrasonic performance. This improves the effectivity of cleaning and makes it possible to remove even the most stubborn contaminants.dry-run protected heating
- temperature selectable by rotary switch; from 30°C to 80°C in increments of 5°C (for H units)
- LED display for heating operation (for H units)
- detachable power cord with IEC plug
- selectable temperature threshold with alarm
- automatic safety shutdown after 8 hours of continuous operation
- automatic safety shutdown at a bath temperature of 90°C

3.2 CE conformity

This Elma ultrasonic cleaner meets the requirements for the CE marking based on the EC/EU Low Voltage, Electromagnetic Compatibility (EMC) and RoHS Directives. Some models are also registered as medical devices.

Refer to the EC/EU Declaration of Conformity that can be obtained from the manufacturer for details.

3.3

RFI Statement (European Union)

This is a Class A product.

Please note:

This equipment has been approved for business purposes with regard to electromagnetic interference.

In a domestic environment this product may cause radio interference in which case the user may be required to take adequate measures.

For this please contact your supplier or the manufacturer of the unit.

3.4

Delivered equipment

- Ultrasonic cleaning unit
- Mains cable
- Operating Instructions
- Stainless-steel cover

3.5

Unit front view / side view

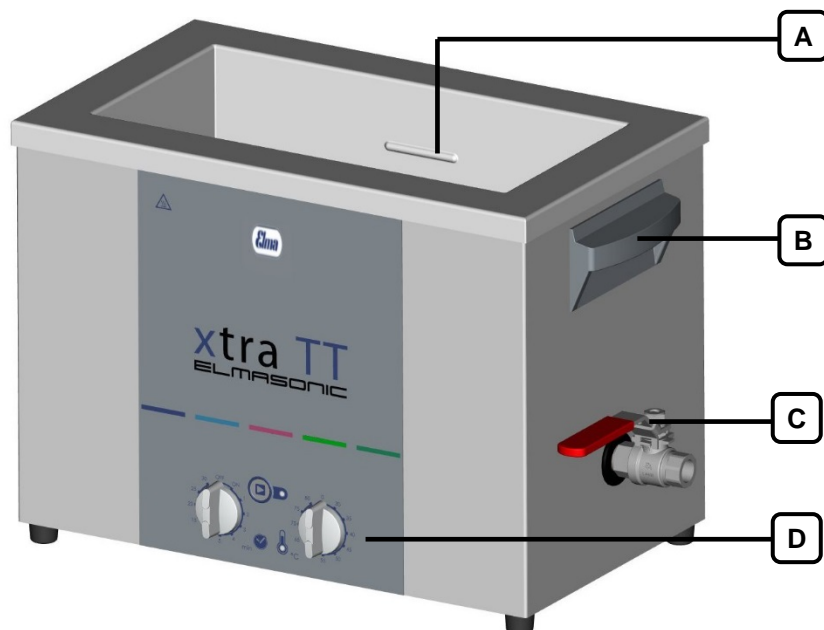


Illustration 4.5: Front view / side view Elma xtra TT 60 H

- A Filling line** indicates the recommended maximum filling level. This level should not be exceeded even with cleaning items inside.
- B Plastic carrying handles** for the safe transportation of the unit even with hot casing.
- C Ball valve for the draining of the tank** functional description see section 3.7.
- D Operating panel** for the control of the operating functions. Description see section 3.8 and 3.9.
- E Stainless-steel cover** to be placed on the tank edge. (*not illustrated*)

3.6

Unit back view

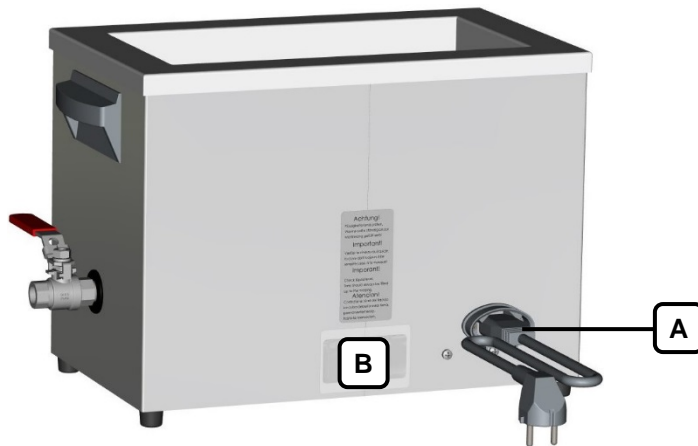


Illustration 4.6: Unit back view

- A Mains supply socket with mains plug** for quick and easy removal of the mains cable e.g. for transportation purposes
- B Name plate** with important information about the unit

3.7

Ball valve for draining the tank

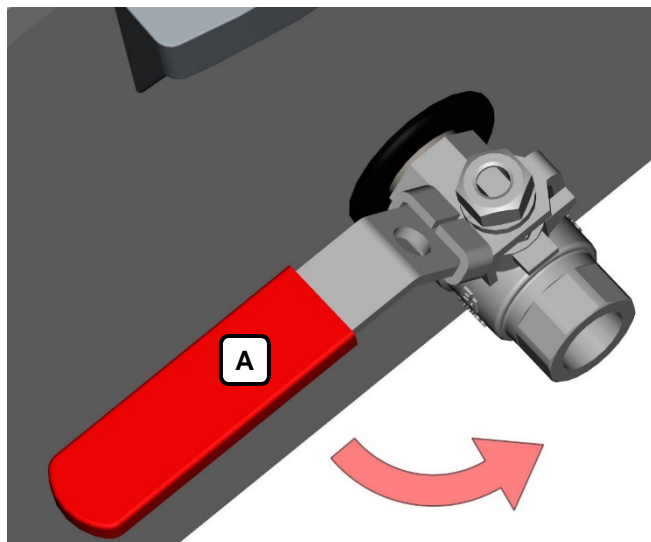


Illustration 4.7: View ball valve for draining the tank

- A Ball valve closed:** Open in direction of the arrow.

3.8

Description of operating elements

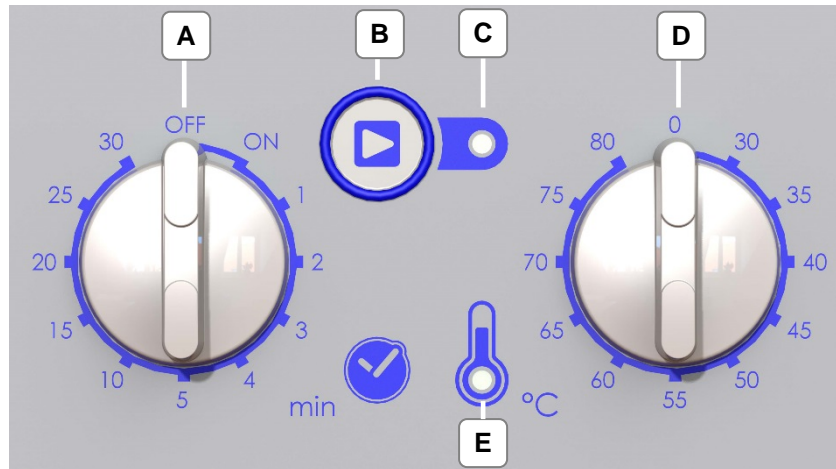


Illustration 4.8: View operating elements (unit with heating)

- A Cleaning time rotary switch** * Setting options Short time operation: 1; 2; 3; 4; 5; 10; 15; 20; 25; 30 min (with automatic switch-off).
Continuous setting ON for continuous operation. The switch-off must be performed manually here.
However, the machine is switched off automatically after 8 hours continuous operation for safety reasons.
 - B Start/Stop button for ultrasound operation**
Activation of the Dynamic mode by pressing and holding for more than 3 seconds.
 - C Ultrasound LED indicator**
Fault indicator (flashes - see *chapter 11*)
 - D Temperature rotary switch** * for machines with heater.
Temperature selection range in 5 °C steps from 30°C – 80°C
 - E Heater LED indicator** for machines with heater,
lights when the heater is active.
Fault indicator (flashes - see *chapter 11*)
- * setting the rotary switch: turn **clockwise**
reset of the rotary switch: turn **anticlockwise**

3.9

Description of LED indicators

Ultrasound operation LED indicator	Device status
off	ultrasound off
lights	ultrasound on (Sweep function) ultrasound time running
flashes slowly (1x/sec)	ultrasound on (Dynamic-mode) ultrasound time running

Heater operation LED indicator	Device status
off	heater off or set point temperature reached
lights	heater is heating
flashes quickly (4x/sec)	specified limit temperature exceeded
lights for approx. 3 seconds, then goes out	temperature limit has been programmed

Ultrasound operation LED indicator and heater operation LED indicator	Device status
pause, flashes 2x, pause...	temperature of liquid too high
pause, flashes 3x, pause...	temperature sensor defective
pause, flashes 4x, pause...	ultrasound power too low
pause, flashes 5x, pause	unknown program error

3.10 Operating and display functions

Action	Input	Result	LED indicator
Switch on machine	Turn cleaning time rotary switch from the "OFF" (12 o'clock) position to the "ON" (1 o'clock) position	Machine operational	no indicator
Start ultrasonic cleaning (sweep mode)	Cleaning time rotary switch \neq "OFF" and Press Start/Stop button briefly	Ultrasound operating for the specified time in sweep mode	Ultrasound LED indicator lights
Start ultrasonic cleaning (Dynamic mode)	Cleaning time rotary switch \neq "OFF" and Press the Start/Stop button for > 2 seconds	Ultrasound operating for the specified time in Dynamic mode	Ultrasound LED indicator flashes slowly
Stop ultrasonic cleaning before expiry	Adjust cleaning time rotary switch or Press Start/Stop button briefly	Ultrasound off	Ultrasound LED indicator off
Switch on heater	Temperature rotary switch not in "0" position and Cleaning time rotary switch \neq "OFF"	Heater LED indicator lights until set point temperature is reached, then extinguishes	

Switch off heater	Temperature rotary switch in the "0" position or Cleaning time rotary switch ≠ "OFF"	Heater LED off	
Program temperature limit	Cleaning time rotary switch in "OFF" position and Temperature rotary switch = desired temperature limit and Press Start/Stop button for > 2 seconds	Specified temperature is programmed (also remains saved after switching off the machine)	The heater LED indicator lights for approx. 3 seconds, then goes out

4 Initial operation

Packing Please keep the original packing or dispose of it according to the relevant waste disposal regulations. You can also return the packing to the manufacturer free destination (to your account).

Check for transport damages Check the unit for possible transport damages before initial operation. In case of visible damage do not connect the unit to the mains. Contact your supplier and forwarding agent.

Placement For operation, place the unit on a dry and solid surface. Ensure that the workplace is sufficiently ventilated! Do not use a soft surface (e.g. a carpet) as this may impede the ventilation of the unit.



DANGER

Risk of electrocution due to humidity inside the unit!
Protect the unit from entering humidity.

The unit inside is splash-water-proof. Keep workplace and casing dry in order to prevent electrical accidents and damages on the unit.

- Ambient conditions**
- Allowed ambient temperature during operation:
+5 °C (+41 °F) to +40 °C (+104 °F)
 - Allowed relative humidity of air during operation: max. 80 %
 - In-door operation only

4.1 Connecting the unit to the mains

Required mains conditions Earth grounded socket:
1 phase (220-240 V); 1 N; 1 PE protective earth.

The power supply must be protected by an earth leakage circuit breaker.

Connect mains cable Use the plug-in mains cable delivered with the unit. Connect the unit to a grounded shockproof socket only. Ensure that the values indicated on the nameplate of the unit correspond with the available connecting conditions.
The mains plug must be connected to an easily accessible socket only, as it serves as interrupted device!

5 Putting unit into operation

5.1 Filling of the unit

Shut the drain Shut the drain duct before filling the tank. (Ball valve - see *section 3.7*).

Observe filling level Fill the cleaning tank with a sufficient quantity of a suitable cleaning liquid before switch-on.



The optimum filling level is approx. 2/3 of the tank volume. The marked maximum filling level of the tank indicates the recommended filling level with cleaning items in the bath (see *also section 4 Illustration 4.5*).

Suitable cleaning agents Ensure that the chosen cleaning agent is suitable for treatment in an ultrasonic bath and observe the instructions on dosage and the compatibility of the material. We recommend the use of the cleaning agents listed in *section 7.3*.

Prohibited cleaning agents Flammable products are generally not allowed for use in an ultrasonic bath. Observe the safety warnings given in *section 7.1*.



DANGER

Risk of fire and explosion!

Never use flammable liquids or solvents directly in an ultrasonic cleaning bath.

Use the cleaning chemicals listed in *section 7.3*.



Ultrasonic activity increases the vaporisation of liquids and creates a very fine mist which can catch fire on any ignition source.

Observe the instructions on limitations of use given in *section 7.1*.



CAUTION

Risk of damage to the transducer tank!

Do not use any acid cleaning agents (pH value < 7) directly in the stainless steel tank if the cleaning items or the contamination of the cleaning items contain halogenides (fluorides, chlorides or bromides). The same applies to NaCl solutions.

Use the cleaning chemicals listed in *section 7.3*.



The stainless steel tank can be destroyed by crevice corrosion in a very short time. Substances that cause crevice corrosion can be contained in household cleaners.

Observe the instructions on limitations of use given in *section 7.2*. For queries please contact the manufacturer or your supplier.



CAUTION

Danger of damage to the transducer system!

Fill no liquid > 60 °C and < 10 °C in the ultrasonic tank.

5.2

Placement of cleaning items

Caution! The ultrasonic bath has been designed for the ultrasonic treatment of items and liquids only.
Do not clean living beings or plants!



Do not reach inside the tank during ultrasonic operation!

Cell walls can be damaged by prolonged exposure to ultrasonic activity.

For placing and taking out the cleaning items always switch off the unit.

No cleaning items on the bottom of the tank

Do not place the cleaning items directly onto the bottom of the cleaning tank, as this might lead to damages to the unit.

Use cleaning basket

Place the cleaning items into the stainless steel cleaning basket (accessory equipment).

Acid tank

For the use of cleaning chemicals which might destroy or damage the stainless steel tank use a separate container. For the special plastic cleaner tank for acid chemicals please contact your supplier.

5.3

Degassing of liquid

Freshly mixed cleaning liquids are saturated with air which lessens the cleaning effect of the ultrasonic activity. By sonification of the liquid over a period of several minutes before the cleaning process the tiny air bubbles in the liquid are eliminated.

How to proceed

1. Adjust the “**Cleaning time rotary switch**” to 5 or 10 minutes.
2. Press the “**Start/Stop button**”.
3. Degas the fresh cleaning liquid for approx. 5 - 10 minutes.

6

Ultrasonic cleaning process

Please observe the following instructions before starting the ultrasonic cleaning process. It is the user's responsibility to check the cleaning results.



CAUTION

Risk of scalding by hot surfaces and cleaning liquid!

Ultrasonic energy is physically transformed into heat.

The unit and the cleaning liquid in the tank heat up during ultrasonic operation even with the heating switched off. During permanent operation with cover temperatures exceeding 60°C can be reached.

During permanent operation with cover and heating temperatures exceeding 80°C can be reached.

Do not reach inside the bath.
If necessary touch unit and basket with protecting gloves!



CAUTION

Ultrasonic units can produce annoying sounds.

Wear personal ear protection devices when working close to an ultrasonic unit which is operated without cover.



ATTENTION

Sensitive surfaces can be damaged when exposed to ultrasound over prolonged periods, particularly at low cleaning frequencies.

Ensure that sensitive surfaces are exposed to ultrasonic activity for a suitable period only.

If in doubt check the cleaning progress regularly and observe the state of the surface material.



ATTENTION

Ultrasonic energy is physically transformed into heat.

The unit and the cleaning liquid in the tank heat up during ultrasonic operation even with the heating switched off. During permanent operation with cover temperatures exceeding 60 °C can be reached.

For the cleaning of temperature-sensitive items please take into consideration the heating-up of the cleaning liquid.

Please observe that the temperature of the cleaning media remains below 42 °C when cleaning parts contaminated with fresh protein or blood.

6.1 Heating up of the cleaning liquid (units with heating)

Depending of the degree and kind of contamination and on the cleaning medium used it might be required to heat up the cleaning liquid. For a quick heating-up process and in order to prevent unnecessary energy losses we recommend to use a cover (optional accessory equipment).



The ultrasonic energy is transformed physically into heat. Low set temperatures can be exceeded during ultrasonic operation.

The cleaning effect through ultrasonic cavitation is reduced when cleaning with high temperatures. We recommend not to exceed a temperature of 80°C inside the tank.

For the recommended cleaning temperature please observe the product information of the used elma clean cleaner.



High temperatures! Risk of burning and scalding!

Cleaning liquid, cleaning tank, casing, cover, basket and cleaning items can heat up considerably.

Do not reach inside the bath.

If necessary wear protective gloves when touching unit and basket!

Cleaning temperature recommendations in the medical sector:

Please observe that the temperature of the cleaning media remains below 42 °C when cleaning parts contaminated with fresh protein or blood.

Please observe the temperature even when using low or no heating.

How to proceed

1. Start the unit with the **“Cleaning time rotary switch”**.
2. Set the desired cleaning temperature at the **“Temperature rotary switch”** for the temperature preselection.
3. The heater is active until the preselected temperature is reached.
4. The LED indicator lights while the heater is active.
5. The LED extinguishes as soon as the preselected temperature is reached.

6.2 Starting the cleaning process manually

- Short time operation**
1. Turn the “**Cleaning time rotary switch**” clockwise to the desired cleaning time for short time operation.
 2. Press the “**Start/Stop button**” to start the ultrasound operation.
 3. The ultrasound is automatically switched off after expiry of the set point time.

Continuous operation Turn the “**Cleaning time rotary switch**” clockwise to the **ON** position for continuous operation. No automatic switch-off is performed in the "Continuous operation". The ultrasound function must be switched off by the user after the cleaning by pressing the “**Start/Stop button**”. Or put the “**Cleaning time rotary switch**” back into the **OFF** position.

ATTENTION Only turn the selector switch anticlockwise back to the 0 position!



Elmasonic xtra TT units are equipped with safety shutdown to prevent inadvertent continuous operation. The machine is completely shut down automatically after 8 hours of continuous operation. If you want to continue operating the machine immediately, you only need to restart it.

6.3 Sweep function

Elmasonic xtra TT units are also equipped with an automatic Sweep function.

How it Works Homogeneous irradiation in the cleaning tank is reached by constant shifting of the maximum zones of the sound pressure.

6.4 **Activate dynamic function**

Special function to intensify the ultrasonic cleaning effect thanks to maximum ultrasonic power and optimised sound field distribution, particularly advantageous for stubborn stains.

How it works Increasing the ultrasonic signal amplitude magnifies the ultrasonic effect. The system repeatedly switches to the sweep function periodically, thus achieving optimised sound field distribution.

- How to proceed**
1. Use the "**Cleaning time rotary switch**" to select the time duration for cleaning.
 2. Press the "**Start/Stop button**" for at least 3 seconds.



This function can also be activated at any time during operation.

6.5 **Programme temperature limit**

This function activates an optical signal when a pre-set temperature limit is reached.

This allows the user to take action in good time to prevent temperature-sensitive items from becoming damaged or from coagulating if blood or egg white is being cleaned.



The LED indicator for heating mode will flash rapidly when the pre-set temperature limit is reached (4 sec.).



ATTENTION

The unit emits an optical signal as a warning only.

The user is responsible for any action required, such as switching off the unit or removing the cleaned item.

- How to proceed**
1. Turn the "**Cleaning time rotary switch**" to "**OFF**".
 2. Turn the "**Temperature rotary switch**" to the required temperature limit.
 3. Press the "**Start/Stop button**" for at least 2 seconds.
 - The heater LED indicator will light up for around 3 seconds.

The pre-set temperature limit is now programmed and will also be stored in the memory when the unit is switched off.

Proceed as follows to delete the programmed temperature limit:

1. Turn the "**Cleaning time rotary switch**" to "**OFF**".
2. Turn the "**Temperature rotary switch**" to "**0**".
3. Press the "**Start/Stop button**" for at least 2 seconds.
 - The heater LED indicator will light up for around 3 seconds.

The pre-set temperature limit is now deleted.

6.6

After the cleaning

Follow-up treatment of cleaning items

When the cleaning process is finished rinse the cleaning items, e.g. under the tap.

Drain the unit

Drain the liquid as soon as it is dirty or when the unit is not operated over a prolonged period of time. Certain residues and types of contamination may destroy or damage the stainless steel tank.

Use the ball valve to drain the cleaning tank
(see section 4.7).

7

Cleaning media



The cleaning chemical to be used must be suitable for the use in an ultrasonic bath to prevent damage to the tank or injuries to the user. Use the recommended cleaners mentioned in *section 8.3*. Observe the restrictions to cleaners containing solvents and aqueous cleaners mentioned in *sections 7.1* and *7.2*.

For queries please contact the manufacturer or your supplier.

Exclusion of liability

Damages caused by non-compliance with the instructions given in *sections 7.1* and *7.2* will not be covered by the manufacturer's warranty!

7.1

Limitations of use of cleaners containing solvents



Never use flammable liquids or solvents directly in an ultrasonic cleaning tank. Risk of fire and explosion!



Ultrasound increases the volume of vaporisation of liquids and creates a very fine mist that can catch fire on any ignition source at any time.

Do **not** fill potentially explosive substances and flammable solvents

- marked in compliance with the EEC directives by symbols and safety warnings R 1 to R 9
- or E, F+, F, O or R 10, R 11 or R 12 for flammable substances

into the stainless steel tank for ultrasonic treatment.

Exception

In compliance with the general regulations on the protection of labour, certain limited volumes of flammable liquids (max. 1 litre) can be used in an ultrasonic cleaning unit under the following conditions: these liquids must be filled into a suitable separate vessel (e.g. beaker) with sufficient ventilation; this vessel (beaker) can then be put into the stainless steel tank which is filled with non-flammable liquid (water with a few drops of surfactant).

7.2

Limitations on aqueous cleaners

Do not use aqueous cleaning media with pH values in the acid range ($\text{pH} < 7$) directly in the ultrasonic tank if fluoride (F^-), chloride (Cl^-) or bromide (Br^-) ions can be taken in by the removed dirt or through the cleaning chemical. These can destroy the stainless-steel tank by crevice corrosion within a very short period of ultrasonic operation.

Acids and alkaline solutions

Other media which can destroy the stainless-steel tanks when used in high concentrations or with high temperatures during ultrasonic operation are: hydrochloric acid, nitric acid, sulphuric acid, formic acid, hydrofluoric acid (even diluted).
(Completeness of list not guaranteed.)

Risk of damage to the unit: do not use cleaning solutions containing more than 0.5 mass % alkali (KOH and/or NaOH) in an ultrasonic cleaning tank.

Entrainment of chemical substances

The above limitations for the use of chemicals in an ultrasonic bath also apply for the aforementioned chemicals when these are brought into an aqueous (particularly distilled water) bath through entrainment or from the removed dirt.

Acid-resistant tank

For the ultrasonic treatment with the above mentioned media use an acid-resistant tank (available as accessory equipment).

Disinfectants

The limitations of use also apply to the standard cleaners and disinfectants if these contain the above mentioned compounds.

Safety regulations

Observe the safety warnings indicated by the manufacturer of the chemicals (e.g. goggles, gloves, R and S phrases).

For queries please contact the manufacturer or your supplier.

7.3

List of recommended cleaning media

Elma has a large range of suitable cleaning products on offer developed by chemical engineers in the Elma laboratory. Please contact your supplier to find the most suitable cleaning chemical for your application.

Environment – friendly products

The organic detergents contained in the elma clean cleaning concentrates are biodegradable. Product informations and safety data sheets are available from the manufacturer.

7.3.1 **Dental**

- elma clean 10** Universal cleaning concentrate for the cleaning of instruments and laboratory equipment made of plastic, ceramic, stainless steel, rubber and glass.
- elma clean 25** Ready-to-use cleaner for impression spoons: removes dental plaster and alginates. Ready-for-use cleaning bath.
- elma clean 35** Cleaning concentrate for prostheses with activated oxygen for the cleaning of dental prostheses made of metal, ceramics and plastic. The released oxygen refreshes the prosthesis hygienically.
- elma clean 40** Chemical cleaning concentrate for the removal of cement and carbonate (lime). For the cleaning of precious metals, ceramics, plastics, glass and rubber. Removes metal oxide, cement, fluxing media, etc.
- elma clean 55d** Aldehyde-free drill cleaning concentrate for instruments made of stainless steel. For the hygienical removal of amalgam remains, blood, tissue, etc.; with anti-corrosion effect.
- elma clean 60** Acid cleaning concentrate for instruments made of stainless steel, glass and plastic. Removes corrosion, rust films and mineral deposits.

7.3.2 **Medical**

- elma clean 10** Universal cleaning concentrate for the cleaning of instruments and laboratory equipment made of plastic, ceramic, stainless steel, rubber and glass.
- elma clean 60** Acid cleaning concentrate for instruments made of stainless steel, glass and plastic. Removes corrosion, rust films and mineral deposits.

7.3.3 **Optics**

- elma opto clean** Cleaning concentrate for glasses, frames, optical lenses and components. Also suitable for plastics.

7.3.4 Laboratory

- elma lab clean S10** Acid cleaning concentrate for glass, ceramics, metal incl. light and non-ferrous heavy metals, plastic. Removes mineral deposits, lime, lime soap and non-ferrous heavy metal oxides, mineral grease and oil.
- elma lab clean S20** Strong acid cleaning concentrate for stainless steel, glass and plastic. Removes tenacious contaminations such as rust, organic residues, inorganic compounds and mineral grease and oil. Not suitable for aluminum and light metal alloys.
- elma lab clean N10** Neutral universal and laboratory cleaning concentrate for sensitive materials such as aluminum and light metals. Removes lime soap, light oil and grease and finger marks.
- elma lab clean A10** Alkaline cleaning concentrate for glass, porcelain, metal and plastic. Removes grease, glass grease, gumming, remains of lables and calcification. Also suitable for the laboratory rinsing machine.
- elma lab clean A20sf** Special cleaning concentrate for pipettes, does not contain any tensides. Mildly alkaline, suitable for use in an ultrasonic cleaning unit and in the laboratory rinsing machine. Also suitable for use in pipette rinsing machines that require active cleaning agents (soaking).

7.3.5 Jewellery

- elma clean 75** Ammoniacal cleaning concentrate with brightening effect for precious and nonferrous heavy metals; for the removal of abrasive and polishing pastes. Not suitable for soft stones, pearls or corals.
- elma clean 85** Gentle, neutral cleaning concentrate for the jewellery workshop. Suitable for soft stones and fancy jewellery.
- elma noble clean** Cleaning and brightening of gold, silver and platinum jewellery within seconds. Not suitable for soft stones, pearls or corals. Ready-to-use cleaner.
- elma ultra clean** Extra gentle, mild alkaline cleaning concentrate for precious metal jewellery, in particular gold and gold-alloys will be given a new shine, with stones. Clean soft stones without ultrasound.
- elma super clean** Ammoniacal cleaning concentrate for jewellery made of precious metals, with brightening effect. Clean soft stones without ultrasound.

7.3.6 Watches

- elma cleaning-concentrate 1:9** Ammoniacal aqueous cleaning concentrate for disassembled watches / clocks with brightening effect on non-ferrous parts.

7.3.7

Industry and workshop

- elma tec clean A1** Cleaning concentrate (alkaline) for electronics and fine optics: removes light oils, grease, fluxing agents, dust, finger prints, etc.
- elma tec clean A2** Intensive cleaner (ammoniacal) with brightening effect for nonferrous and precious metals: removes grinding, polishing and lapping media, grease, oil, etc.
- elma tec clean A3** Cleaning concentrate (alkaline) for iron, steel, stainless steel and precious metals: removes punching oil, drawing grease, soot, forge, grinding and polishing media, high-performance cooling lubricants, etc.
- elma tec clean A4** Universal cleaning concentrate (alkaline): removes oil, grease, soot, coking, forge, dust, finger prints, etc.
- elma tec clean A5** Powerful cleaner (alkaline) in powder form for iron and light metals: removes forged and gummed oil and grease, grinding and polishing media, lacquer and paint remnants, wax, etc.
- elma tec clean N1** Neutral cleaning concentrate: removes oil, grease, grinding, lapping and polishing media, dust, sweat, finger prints, etc.
- elma tec clean S1** Mild acid cleaning concentrate: removes rust, lime, oxide films (e.g. verdigris), grease, oil, etc.
- elma tec clean S2** Strong acid cleaning concentrate: removes mineral contaminations such as lime, rust and other oxides, films that can be removed with corrosives, etc.

8 Maintenance

8.1 Maintenance / Care



ATTENTION

Electrical security

Pull the mains plug before carrying out any maintenance works!

The present Elmasonic unit is maintenance-free. Check the casing and the mains cable for damage regularly in order to prevent electrical accidents.

Care of transducer tank

Lime deposits on the stainless-steel tank can be cleaned gently e.g. with elma clean 40 or elma clean 115C (operate the unit with concentrate + water).

Grid of air fan

Check regularly the grid of the air fan at the bottom of the unit (not existent in all units).

Remove dirt if necessary to allow sufficient ventilation inside the unit.

Care of casing

Residues of cleaning media can be wiped away with a household cleaner or decalcifier depending on the kind of contamination. **Do not put the unit in or under water!**

Disinfection

If the unit is used for medical and sanitary purposes it is necessary to disinfect the transducer tank and the surfaces regularly (standard surface disinfectants).

8.2

Service life of the transducer tank



The transducer tank and particularly the ultrasound transmitting surfaces are wear parts. The changes on the surfaces that occur after a certain operating period are visible first as grey areas and later on as material abrasions, the so-called cavitation erosion.

To prolong the service life of your ultrasonic unit even more we recommend to observe the following instructions:

- Regularly remove any cleaning residues, in particular metal particles and rust films.
- Use suitable cleaning chemicals, with particular caution concerning the kind of removed contamination (see instructions *section 7.2*).
- Abrasive particles from removed contaminations (e.g. polishing pastes) must be drained and removed from the cleaning tank as frequently as possible (exchange the cleaning bath).
- Exchange the cleaning medium before it is too heavily contaminated.
- Do not operate the ultrasound unnecessarily; switch off after the cleaning process.

8.3

Repair

**Opening by authorised
specialised personnel
only**

Repair and maintenance works which require the unit to be connected and opened must be carried out by authorised and specialised personnel only.



Risk of electrocution due to live parts inside the unit!

Pull the mains plug before opening the unit!

The manufacturer cannot be held responsible for any damage caused by unauthorised maintenance or repair works on the unit.

In the case of a break-down of the unit, please contact the manufacturer or your supplier.

9 Technical Details

Elmasonic xtra TT	30H	60H	120H	200H
Mechanical data				
Max. volume of trough (L)	3	6,5	14	18
Working volume of trough (L)	2	5	10	13
Internal dimensions of trough W x D x H (approximate in mm)	240x130x100	300x150x150	300x240x200	320x280x200
External dimensions of device W x D x H (approximate in mm)	360x230x250	420x250x300	440x340x350	420x390x330
Weight (kg)	6	10	11	13
Max. basket loading (kg)	1	3	7	8
Ball valve (")	3/8	3/8	3/8	3/8
Electrical data				
Mains voltage (Vac)	115-120 220-240	115-120 220-240	115-120 220-240	115-120 220-240
Ultrasound frequency (kHz)	37	37	37	37
Total power consumption (W)	540	550	1000	1500
Effective ultrasound output (W)	140	150	200	300
Max. peak ultrasound output * (W)	560	600	800	1200
Heating power (W)	400	400	800	1200

Technical Details

Accessories				
Stainless steel basket * (W x D x H) mm	216x106x48	276x126x76	271x214x136	291x254x130
Noise level				
Sound pressure level (L_{pAU})**	<80 dB			
Ultrasound level (L_{pZ})***	<100 dB			

* Due to the signal shape, four times the value results for the maximum peak value of ultrasound output.

*** Measured sound pressure level with basket and noise protection cover at a distance of 1 meter.

10 Troubleshooting

Problem	Possible cause	Remedy
Case damaged	<ul style="list-style-type: none"> External influence, transport damage 	<ul style="list-style-type: none"> Send machine to the supplier or manufacturer
Mains power cable damaged	<ul style="list-style-type: none"> External influence, transport damage 	<ul style="list-style-type: none"> Obtain original mains power cable from manufacturer or supplier
No machine functions; All LED indicators dark	<ul style="list-style-type: none"> Mains plug not plugged in 	<ul style="list-style-type: none"> Plug in the mains plug
	<ul style="list-style-type: none"> De-energised power socket 	<ul style="list-style-type: none"> Check power socket / fuse
	<ul style="list-style-type: none"> Mains power cable damaged / interrupted 	<ul style="list-style-type: none"> Replace mains power cable
	<ul style="list-style-type: none"> Electronics fault 	<ul style="list-style-type: none"> Send machine to manufacturer / supplier
No ultrasound function; ultrasound LED indicator dark	<ul style="list-style-type: none"> Cleaning time rotary switch in "OFF" position 	<ul style="list-style-type: none"> Put cleaning time rotary switch in "ON" position
	<ul style="list-style-type: none"> Start/stop button not pressed 	<ul style="list-style-type: none"> Press start/stop button
	<ul style="list-style-type: none"> Electronics fault 	<ul style="list-style-type: none"> Send machine to manufacturer / supplier
Cleaning result not satisfactory	<ul style="list-style-type: none"> Possibly no or unsuitable cleaning agent 	<ul style="list-style-type: none"> Use appropriate cleaning agent
	<ul style="list-style-type: none"> Cleaning temperature may not be optimal 	<ul style="list-style-type: none"> Heat cleaning liquid
	<ul style="list-style-type: none"> Cleaning time may be too short 	<ul style="list-style-type: none"> Repeat cleaning interval

Problem	Possible cause	Remedy
Machine does not heat up; LED temperature indicator dark	<ul style="list-style-type: none"> • Temperature rotary switch in "0" position. 	<ul style="list-style-type: none"> • Adjust a temperature with the temperature rotary switch.
	<ul style="list-style-type: none"> • Machine is switched off 	<ul style="list-style-type: none"> • Put cleaning time rotary switch in "ON" position
	<ul style="list-style-type: none"> • Electronics fault 	<ul style="list-style-type: none"> • Send machine to manufacturer / supplier
Heating up time not satisfactory	<ul style="list-style-type: none"> • Heat energy escapes 	<ul style="list-style-type: none"> • Use cover (optional accessory)
	<ul style="list-style-type: none"> • No circulation of the cleaning liquid 	<ul style="list-style-type: none"> • e.g. also switch on ultrasound
Machine produces cooking noises during heating	<ul style="list-style-type: none"> • No circulation of the cleaning liquid 	<ul style="list-style-type: none"> • e.g. also switch on ultrasound
Specified temperature is exceeded	<ul style="list-style-type: none"> • Temperature sensor is not measuring the average temperature (no circulation) 	<ul style="list-style-type: none"> • Circulate liquid manually or with ultrasound
	<ul style="list-style-type: none"> • Temperature preselection too low 	<ul style="list-style-type: none"> • Do not use heater for low set point temperatures
	<ul style="list-style-type: none"> • Ultrasound energy continues to heat the liquid (physical process) 	<ul style="list-style-type: none"> • Only switch on ultrasound for a short time
LED indicators	pause, flashes 2x, pause...	temperature of liquid too high
LED indicators	pause, flashes 3x, pause...	temperature sensor defective
LED indicators	pause, flashes 4x, pause...	ultrasound power too low
LED indicators	pause, flashes 5x, pause...	unknown program error

11



Putting out of action and waste disposal

The machine components can be disposed of through electronics and metal recycling facilities. The manufacturer also accepts old components for disposal.

12



Australian & New Zealand Distribution:

TECHSPAN GROUP

SYDNEY - BRISBANE - AUCKLAND

Australia:

P. 1-800 148 791

E. info@elma-ultrasonic.com.au

www.elma-ultrasonic.com.au

New Zealand:

P. (09) 827 6567

E. info@elma-ultrasonic.co.nz

www.elma-ultrasonic.co.nz

Technical Support

Australia:

P. 1-800 148 791

E. info@elma-ultrasonic.com.au

www.elma-ultrasonic.com.au

New Zealand:

P. (09) 827 6567

E. info@elma-ultrasonic.co.nz

www.elma-ultrasonic.co.nz